



CONTACT


Thomas Proffen
505-665-6573
505-665-2676 (fax)
tproffen@lanl.gov

The Neutron Powder Diffractometer (NPDF) is a high-resolution total-scattering powder diffractometer located at Flight Path 1, 32 meters from the spallation neutron target. It comprises 20 detector panels with a total of 160 position-sensitive detectors in the backscattering region of the instrument. NPDF is designed for pair distribution function (PDF) studies of disordered and nanocrystalline materials, but it is equally well-suited for high-resolution crystallographic studies. The instrument is available to general users.

On September 27, 2002, the shutter of NPDF opened for the first time. During the rest of the 2002 run cycle, NPDF produced over 300 experimental data sets. An example of


a PDF of nickel extending out

to a distance of $r = 100 \text{ \AA}$ is shown below. (A standard data set suitable for PDF analysis can be obtained in only two hours.) These promising results put NPDF at the cutting edge of local structure determination and also serve as a development platform for this new structure analysis tool for disordered and nanostructured materials.

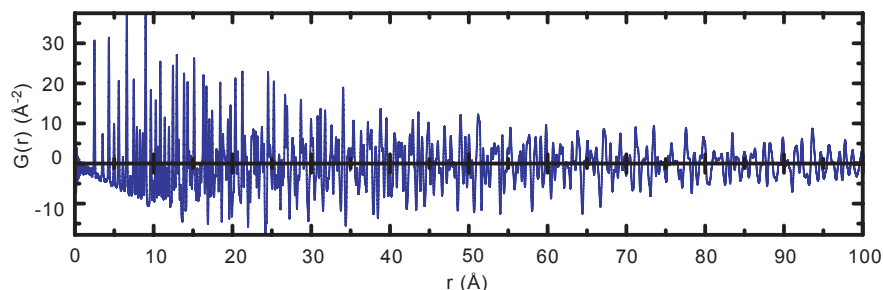

PDF of nickel extending out to a distance of $r = 100 \text{ \AA}$.

The NPDF project was funded by the National Science Foundation; University of Pennsylvania; Michigan State University; University of California at Santa Barbara; University of Virginia; and State University of New York at Stony Brook, as well as Los Alamos National Laboratory.

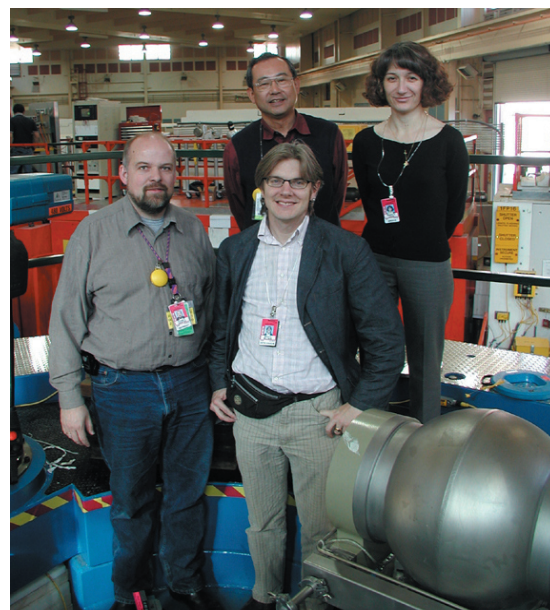

Pictured are some of the sponsors of NPDF: Top row, left to right: Takeshi Egami, University of Pennsylvania, and Despina Louca, University of Virginia. Bottom row, left to right: Thomas Proffen, LANSCE-12, and Simon Billinge, Michigan State University.

Not shown are John Parise, State University of New York at Stony Brook, and Tony Cheetham, University of California at Santa Barbara.

General Information			
Moderator	chilled water (283 K)		
Flight path	primary: 32 m, secondary: 1.5 m		
Beam size	5-cm high x 1-cm wide		
Detector Bank Information			
Bank	90	119	148
d-spacing	0.17–4.2 Å	0.14–3.4 Å	0.12–3.0 Å
Q	1.5–37.6 Å ⁻¹	1.8–45.8 Å ⁻¹	2.1–51.1 Å ⁻¹
Measured d/d	0.31%	0.28%	0.15%
Detector type	124 ³ He tubes	80 ³ He PSDs	80 ³ He PSDs
Pixels	124	4000	4000
Pixel size (w x h)	0.5" x 12"	0.5" x 1.0"	0.5" x 1.0"
Ancillary Equipment			
Displex	15–320 K (closed cycle refrigerator)		
Furnace	ambient - 1200°C		
Other	special furnaces, xyz translation table cryostat contact instrument scientist		